

TM-VI-252, Na+

7.926  
7.806  
7.670  
7.404  
7.385  
7.365  
7.193  
7.174  
7.156

4.911  
4.251  
4.234  
4.216  
4.198  
3.368  
3.329

1.352  
1.334  
1.317


**Av-400C**

Current Data Parameters  
 NAME Jan24-2022  
 EXPNO 70  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20220124  
 Time 17.14  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB/  
 PULPROG zg30  
 TD 32768  
 SOLVENT MeOD  
 NS 16  
 DS 2  
 SWH 8012.820 Hz  
 FIDRES 0.244532 Hz  
 AQ 2.0447233 sec  
 RG 199.33  
 DW 62.400 usec  
 DE 6.50 usec  
 TE 294.6 K  
 D1 1.00000000 sec  
 TD0 1

===== CHANNEL f1 =====  
 SFO1 400.2024012 MHz  
 NUC1 1H  
 P1 11.25 usec  
 PLW1 19.95299911 W

F2 - Processing parameters  
 SI 32768  
 SF 400.2000000 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00

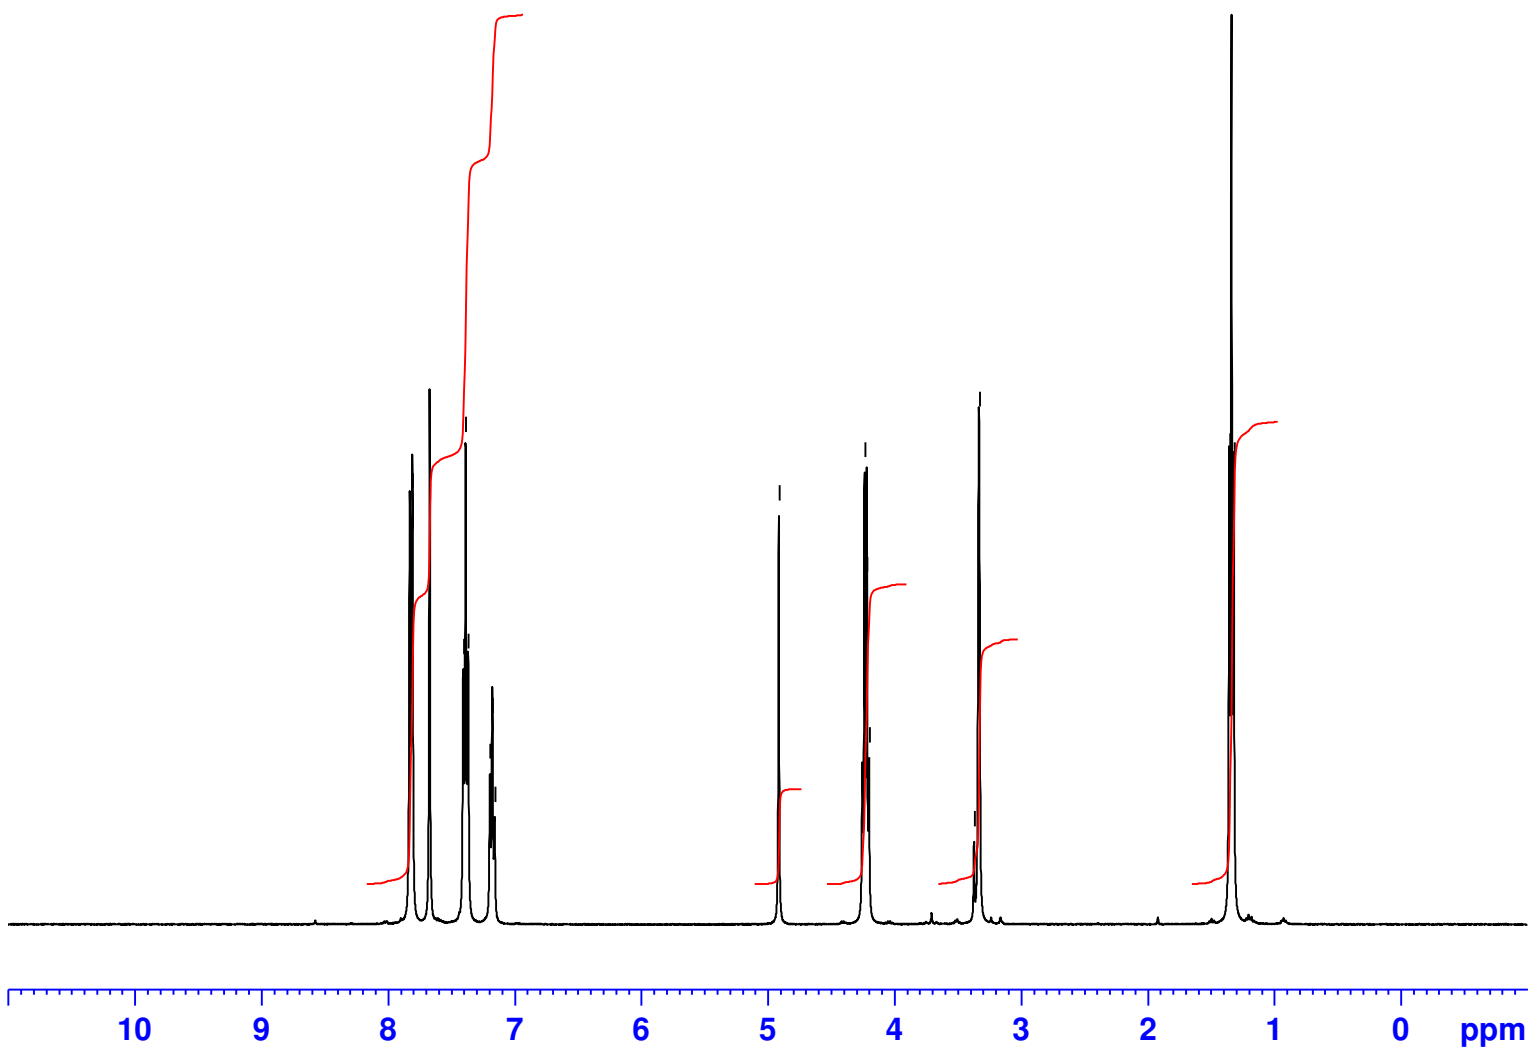

44.09  
4.82  
15.22  
12.41  
23.46