


**Av-400C**

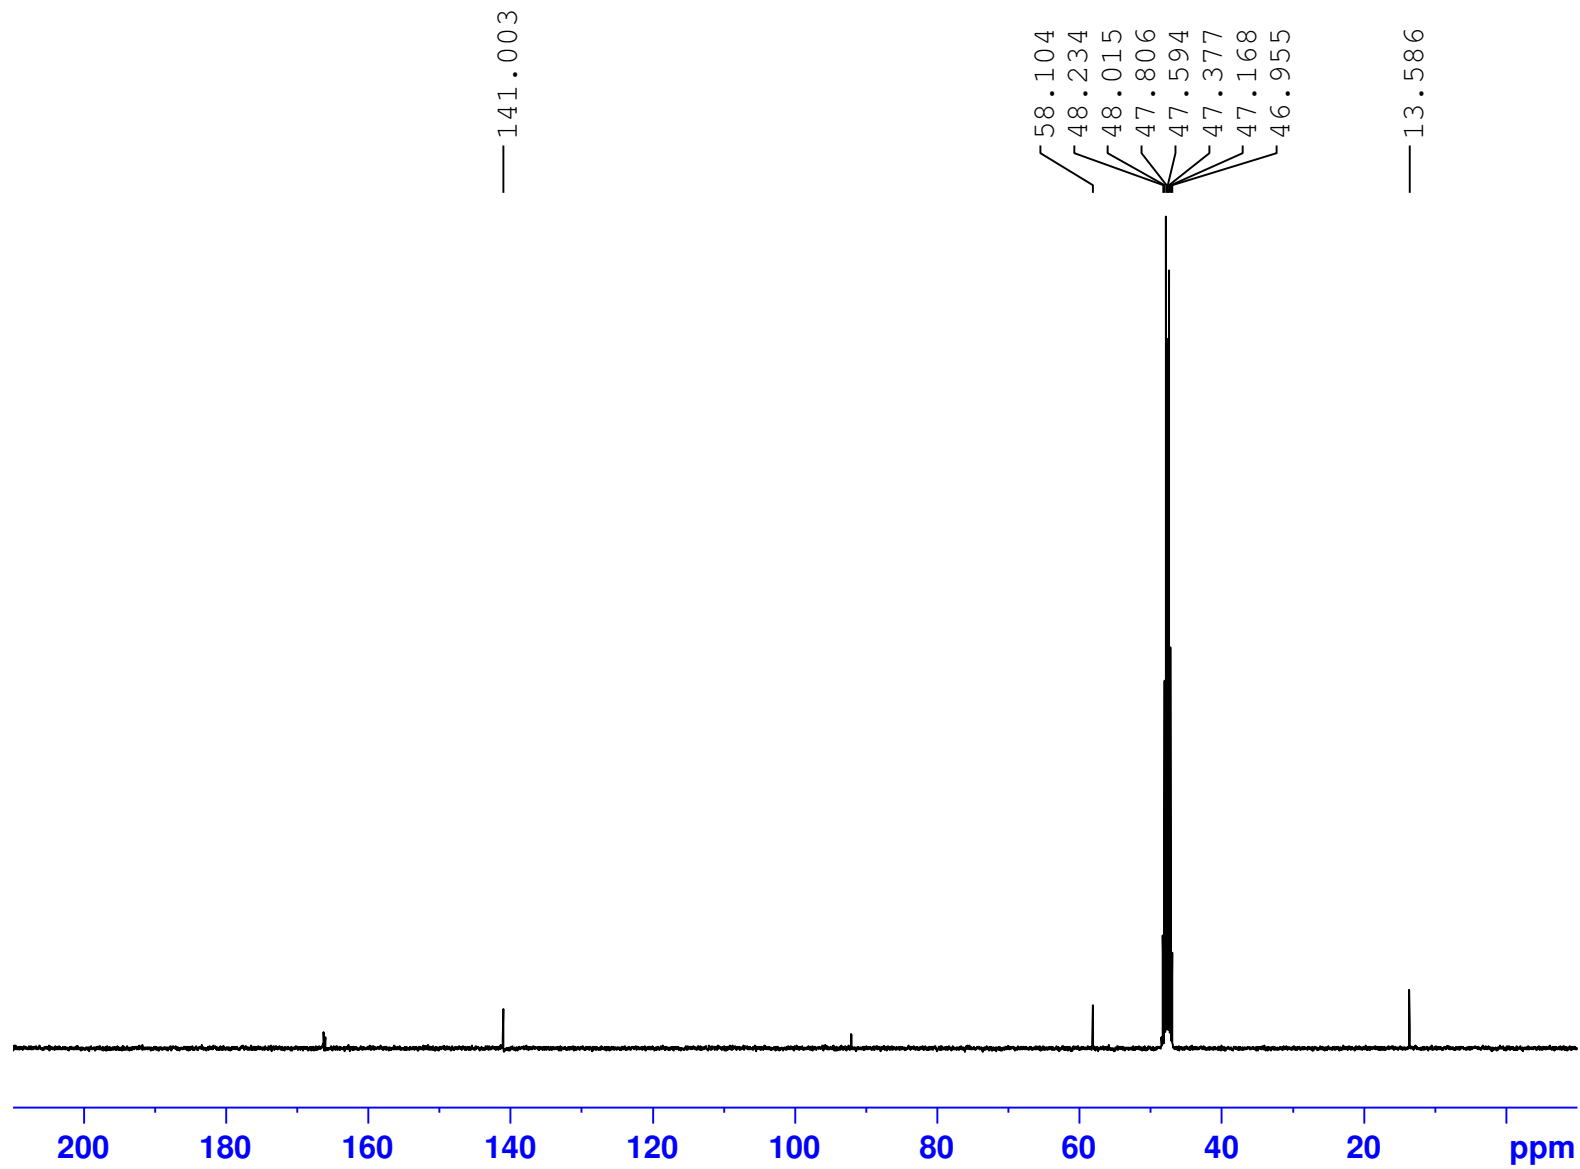

58.104  
48.234  
48.015  
47.806  
47.594  
47.377  
47.168  
46.955

141.003

13.586

Current Data Parameters  
NAME Jan24-2022  
EXPNO 93  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220125  
Time 0.54  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgpg30  
TD 32768  
SOLVENT MeOD  
NS 1200  
DS 4  
SWH 28409.092 Hz  
FIDRES 0.866977 Hz  
AQ 0.5767168 sec  
RG 199.33  
DW 17.600 usec  
DE 6.50 usec  
TE 296.0 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 100.6414395 MHz  
NUC1 13C  
P1 9.05 usec  
PLW1 60.25600052 W

==== CHANNEL f2 =====  
SFO2 400.2020010 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 19.95299911 W  
PLW12 0.33147001 W  
PLW13 0.26848999 W

F2 - Processing parameters  
SI 16384  
SF 100.6303700 MHz  
WDW EM  
SSB 0  
LB 2.00 Hz  
GB 0  
PC 1.40