Agilent Technologies

Sample ID:TM-VI-112
Sample Scans:60
Background Scans:24
Resolution:2
System Status:Good

Method Name:agmb_default2
User:Admin
Date/Time:10/12/2021 12:15:42 PM
Range:4000 - 500
Apodization:Happ-Genzel
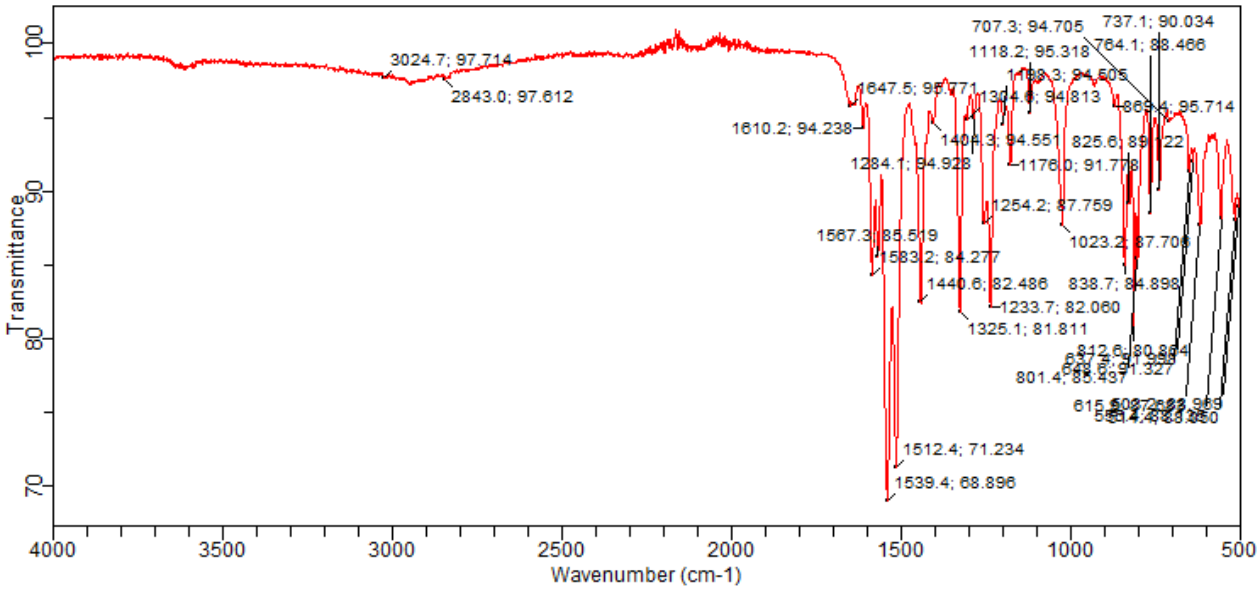
File Location:C:\Users\Public\Documents\Agilent\MicroLab\Results\\TM-VI-112_2021-10-12T12-15-42.a2r