


**Av-400A**

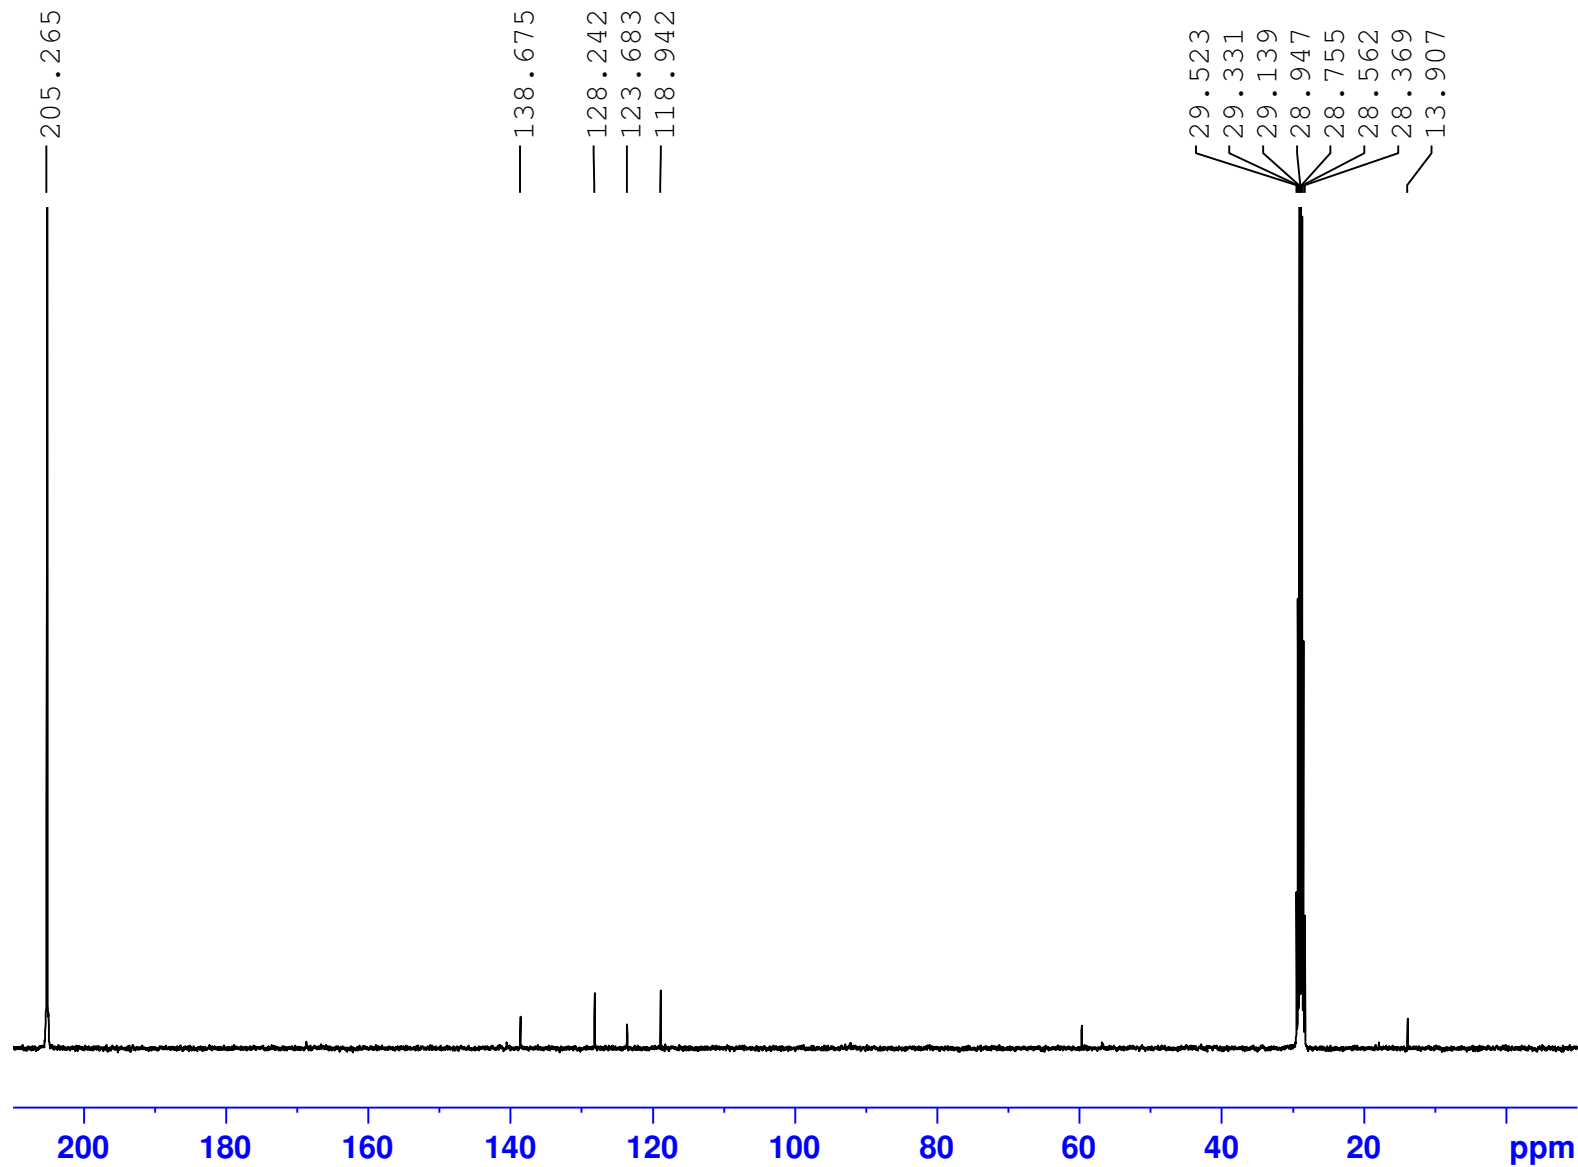

Current Data Parameters  
 NAME Oct20-2021  
 EXPNO 51  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20211020  
 Time 21.11  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB/  
 PULPROG zgpg30  
 TD 32768  
 SOLVENT Acetone  
 NS 1200  
 DS 4  
 SWH 26315.789 Hz  
 FIDRES 0.803094 Hz  
 AQ 0.6225920 sec  
 RG 207.33  
 DW 19.000 usec  
 DE 6.50 usec  
 TE 294.9 K  
 D1 1.00000000 sec  
 D11 0.03000000 sec  
 TD0 1

==== CHANNEL f1 =====  
 SFO1 100.6942485 MHz  
 NUC1 13C  
 P1 9.60 usec  
 PLW1 59.97900009 W

==== CHANNEL f2 =====  
 SFO2 400.4119220 MHz  
 NUC2 1H  
 CPDPRG[2] waltz16  
 PCPD2 90.00 usec  
 PLW2 19.95299911 W  
 PLW12 0.31176999 W  
 PLW13 0.25253001 W

F2 - Processing parameters  
 SI 16384  
 SF 100.6831750 MHz  
 WDW EM  
 SSB 0  
 LB 2.50 Hz  
 GB 0  
 PC 1.40