

TM-VI-169 acetone-d₆ pyr.

7.645
7.501
7.409
7.385
7.267
6.959

4.985

3.689
3.621
3.607
3.591
3.574
3.557
3.471
3.023

2.070
2.066

1.150
1.132
1.115


Av-400C

Current Data Parameters
 NAME Nov18-2021
 EXPNO 50
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20211118
 Time 13.19
 INSTRUM spect
 PROBHD 5 mm PABBO BB-
 PULPROG zg30
 TD 32768
 SOLVENT Acetone
 NS 16
 DS 2
 SWH 8012.820 Hz
 FIDRES 0.244532 Hz
 AQ 2.0447233 sec
 RG 199.33
 DW 62.400 usec
 DE 6.50 usec
 TE 294.6 K
 D1 1.00000000 sec
 TD0 1

==== CHANNEL f1 =====
 SFO1 400.2024012 MHz
 NUC1 1H
 P1 10.00 usec
 PLW1 19.95299911 W

F2 - Processing parameters
 SI 32768
 SF 400.2000000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

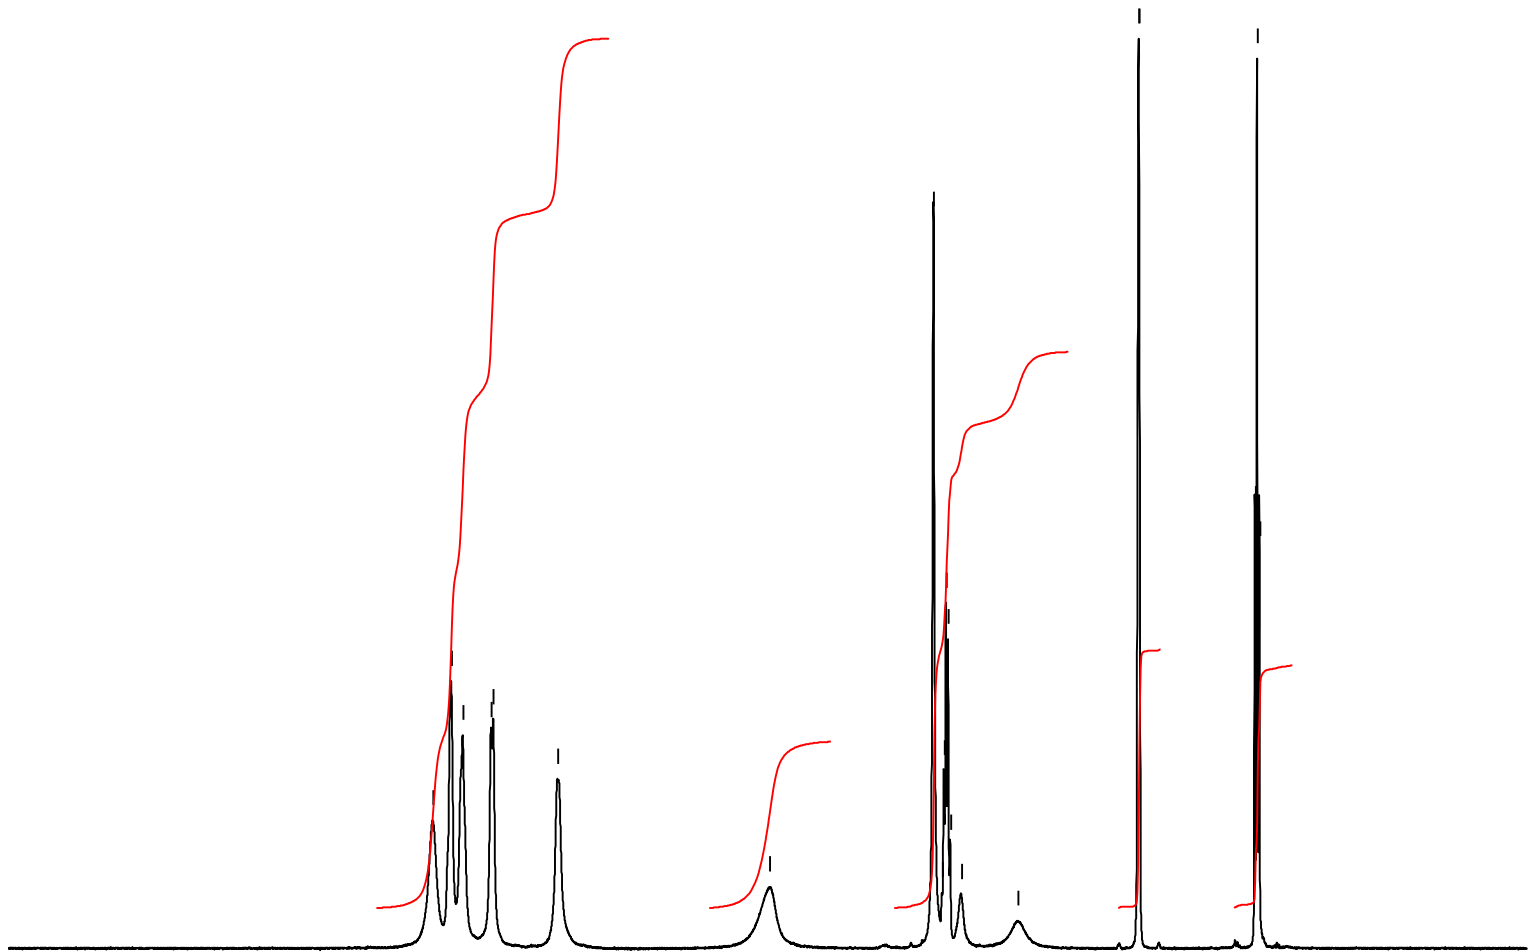

10 9 8 7 6 5 4 3 2 1 0 ppm

41.52

7.95

26.57

12.36

11.60