

TM-VI-108solid Ca+pmb5
 7.344
 7.167
 7.147
 6.882
 6.662
 batch 2

4.913
 3.960
 3.944
 3.771
 3.700
 3.587
 3.570
 3.553
 3.474
 2.977
 2.072
 2.068
 1.306
 1.150
 1.132
 1.114
 1.094


Av-400C

Current Data Parameters
 NAME Oct20-2021
 EXPNO 20
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20211020
 Time 15.58
 INSTRUM spect
 PROBHD 5 mm PABBO BB-
 PULPROG zg30
 TD 32768
 SOLVENT Acetone
 NS 16
 DS 2
 SWH 8012.820 Hz
 FIDRES 0.244532 Hz
 AQ 2.0447233 sec
 RG 177.81
 DW 62.400 usec
 DE 6.50 usec
 TE 294.4 K
 D1 1.00000000 sec
 TD0 1

===== CHANNEL f1 =====
 SFO1 400.2024012 MHz
 NUC1 1H
 P1 10.00 usec
 PLW1 19.95299911 W

F2 - Processing parameters
 SI 32768
 SF 400.2000000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

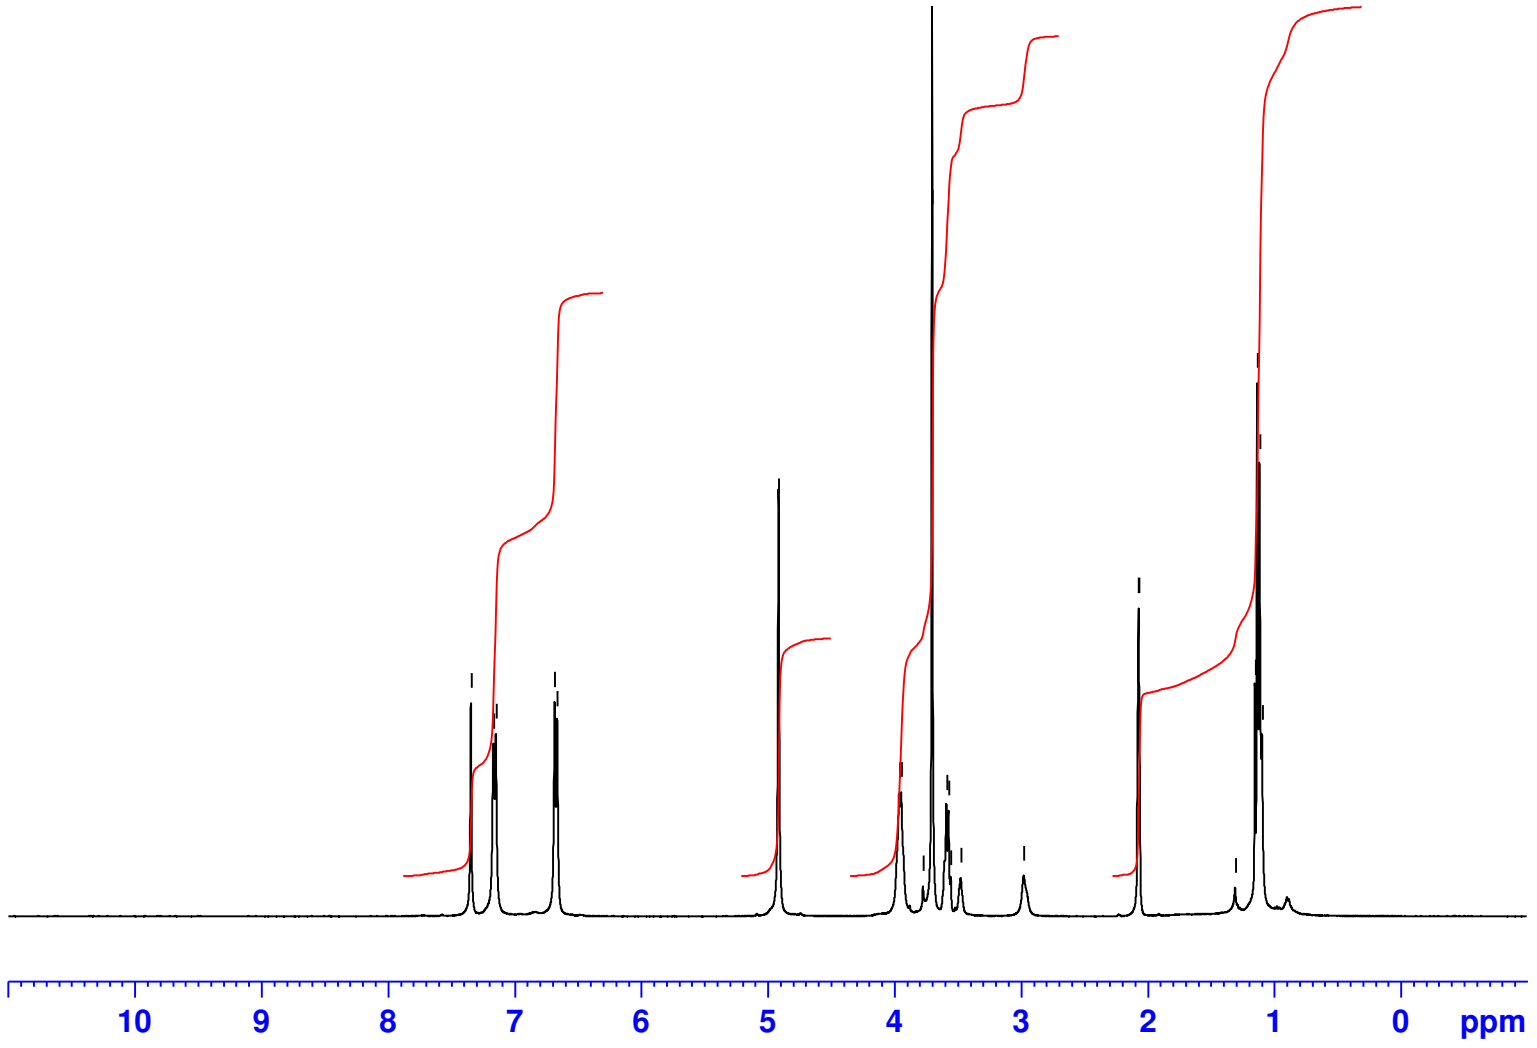

23.05
 9.40
 33.20
 34.36