

TM-VI-107solid

8.176  
8.155  
7.558  
7.523  
7.504  
7.484  
7.480  
7.462  
7.044

4.224  
4.207  
4.189  
4.171  
3.615  
3.598  
3.581  
3.564  
3.021

2.067  
1.287  
1.270  
1.252  
1.153  
1.136  
1.118


**Av-400C**

Current Data Parameters  
 NAME Oct20-2021  
 EXPNO 30  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20211020  
 Time 16.01  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB-  
 PULPROG zg30  
 TD 32768  
 SOLVENT Acetone  
 NS 16  
 DS 2  
 SWH 8012.820 Hz  
 FIDRES 0.244532 Hz  
 AQ 2.0447233 sec  
 RG 199.33  
 DW 62.400 usec  
 DE 6.50 usec  
 TE 294.4 K  
 D1 1.00000000 sec  
 TD0 1

==== CHANNEL f1 =====  
 SFO1 400.2024012 MHz  
 NUC1 1H  
 P1 10.00 usec  
 PLW1 19.95299911 W

F2 - Processing parameters  
 SI 32768  
 SF 400.2000000 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00

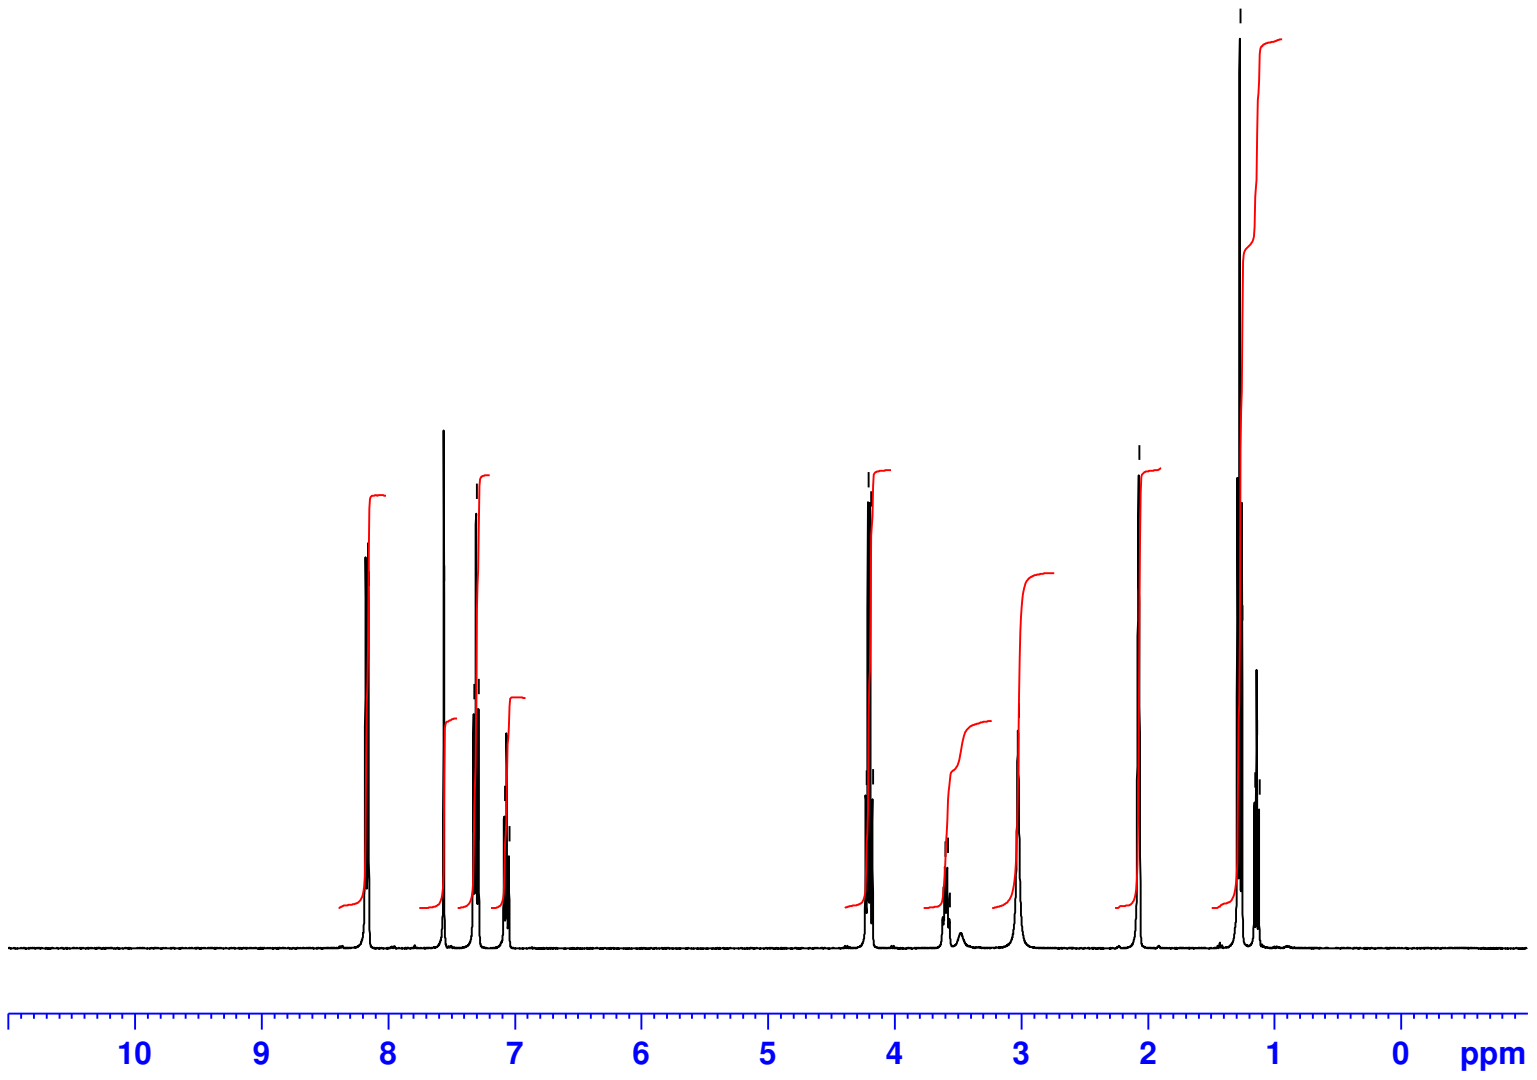

11.74  
5.40  
12.32  
5.98  
12.47  
5.33  
9.53  
12.51  
24.72