

TM-VI-170

ac
 7.6773
 7.6555
 7.6007
 7.4889
 7.4771
 7.4226
 7.4108
 7.3990
 7.3111
 7.1190
 6.6550
 6.6330

4.931
 3.676
 3.620
 3.603
 3.587
 3.570
 3.552
 3.433
 3.420
 3.408
 2.891
 2.858
 2.068
 1.151
 1.133
 1.116


Av-400C

Current Data Parameters
 NAME Nov18-2021
 EXPNO 60
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20211118
 Time 13.23
 INSTRUM spect
 PROBHD 5 mm PABBO BB-
 PULPROG zg30
 TD 32768
 SOLVENT Acetone
 NS 16
 DS 2
 SWH 8012.820 Hz
 FIDRES 0.244532 Hz
 AQ 2.0447233 sec
 RG 199.33
 DW 62.400 usec
 DE 6.50 usec
 TE 294.6 K
 D1 1.00000000 sec
 TD0 1

===== CHANNEL f1 =====
 SFO1 400.2024012 MHz
 NUC1 1H
 P1 10.00 usec
 PLW1 19.95299911 W

F2 - Processing parameters
 SI 32768
 SF 400.2000000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

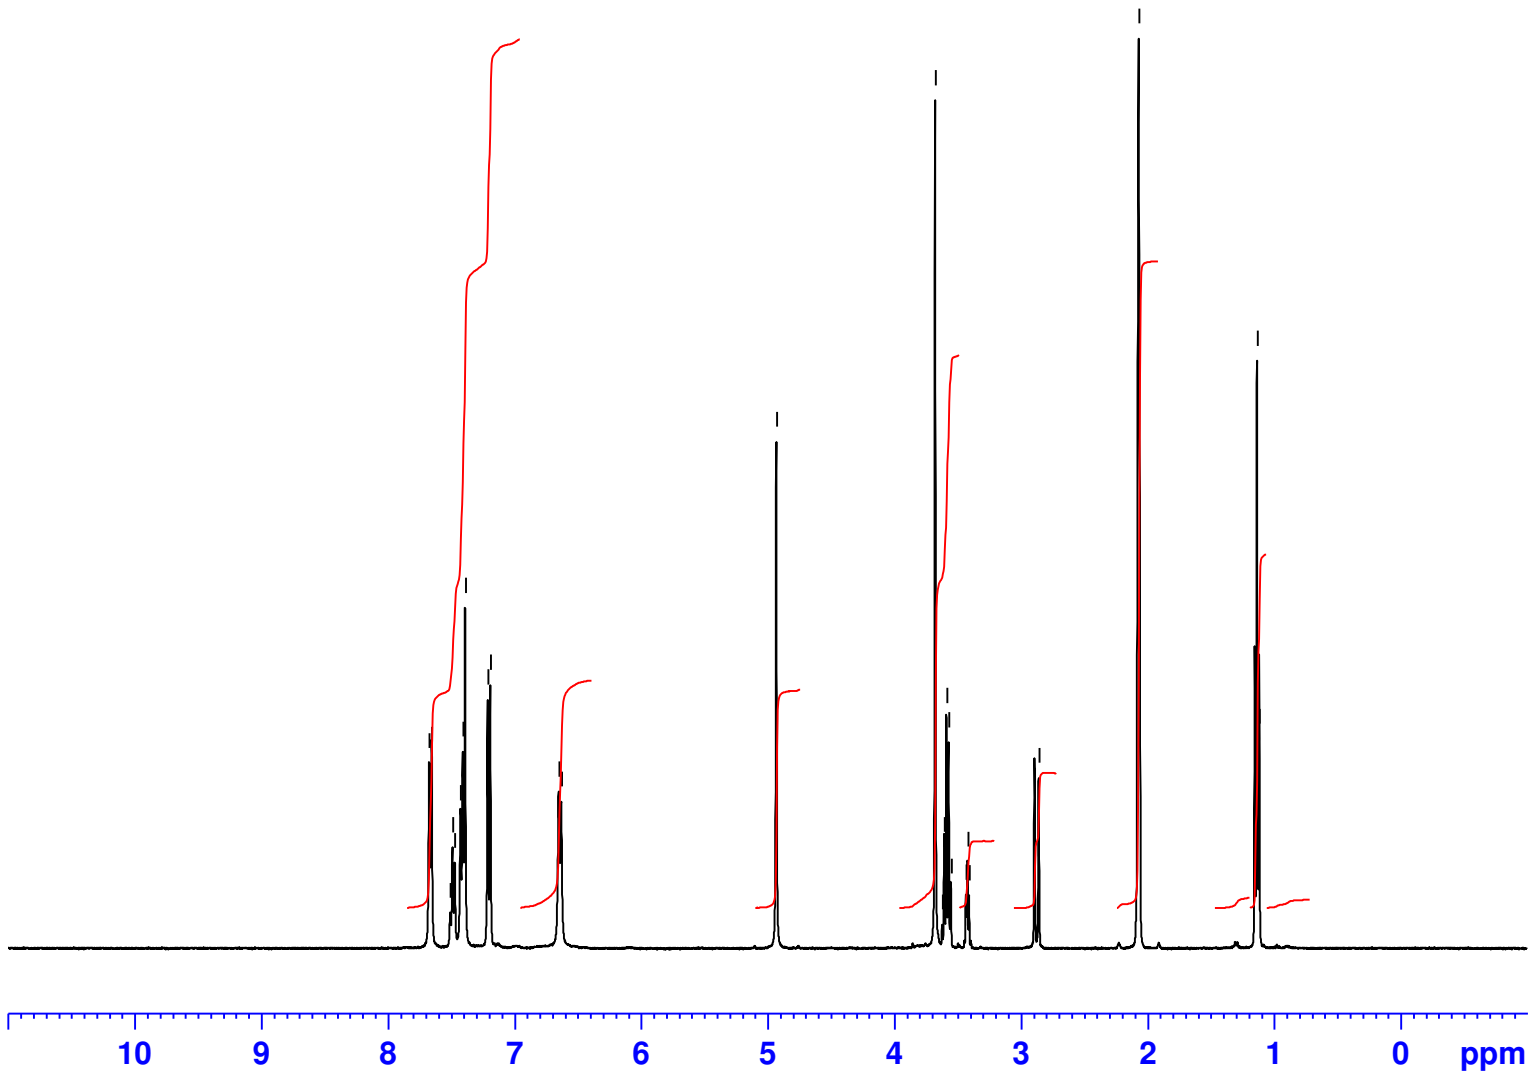

28.13
 7.36
 7.07
 17.91
 2.17
 4.36
 20.94
 0.34
 11.45
 0.26