

TM-VI-136solid

7.917
7.898
7.780
7.390
7.371
7.352
7.286
7.233
7.216
7.198

4.378
4.361
4.344
4.327

1.761
1.391
1.374
1.357
1.284
1.195
0.886


Av-400C

Current Data Parameters
 NAME Oct25-2021
 EXPNO 40
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20211025
 Time 16.00
 INSTRUM spect
 PROBHD 5 mm PABBO BB-
 PULPROG zg30
 TD 32768
 SOLVENT CDCl3
 NS 16
 DS 2
 SWH 8012.820 Hz
 FIDRES 0.244532 Hz
 AQ 2.0447233 sec
 RG 142.23
 DW 62.400 usec
 DE 6.50 usec
 TE 293.2 K
 D1 1.00000000 sec
 TD0 1

==== CHANNEL f1 =====
 SFO1 400.2024012 MHz
 NUC1 1H
 P1 10.00 usec
 PLW1 19.95299911 W

F2 - Processing parameters
 SI 32768
 SF 400.2000000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

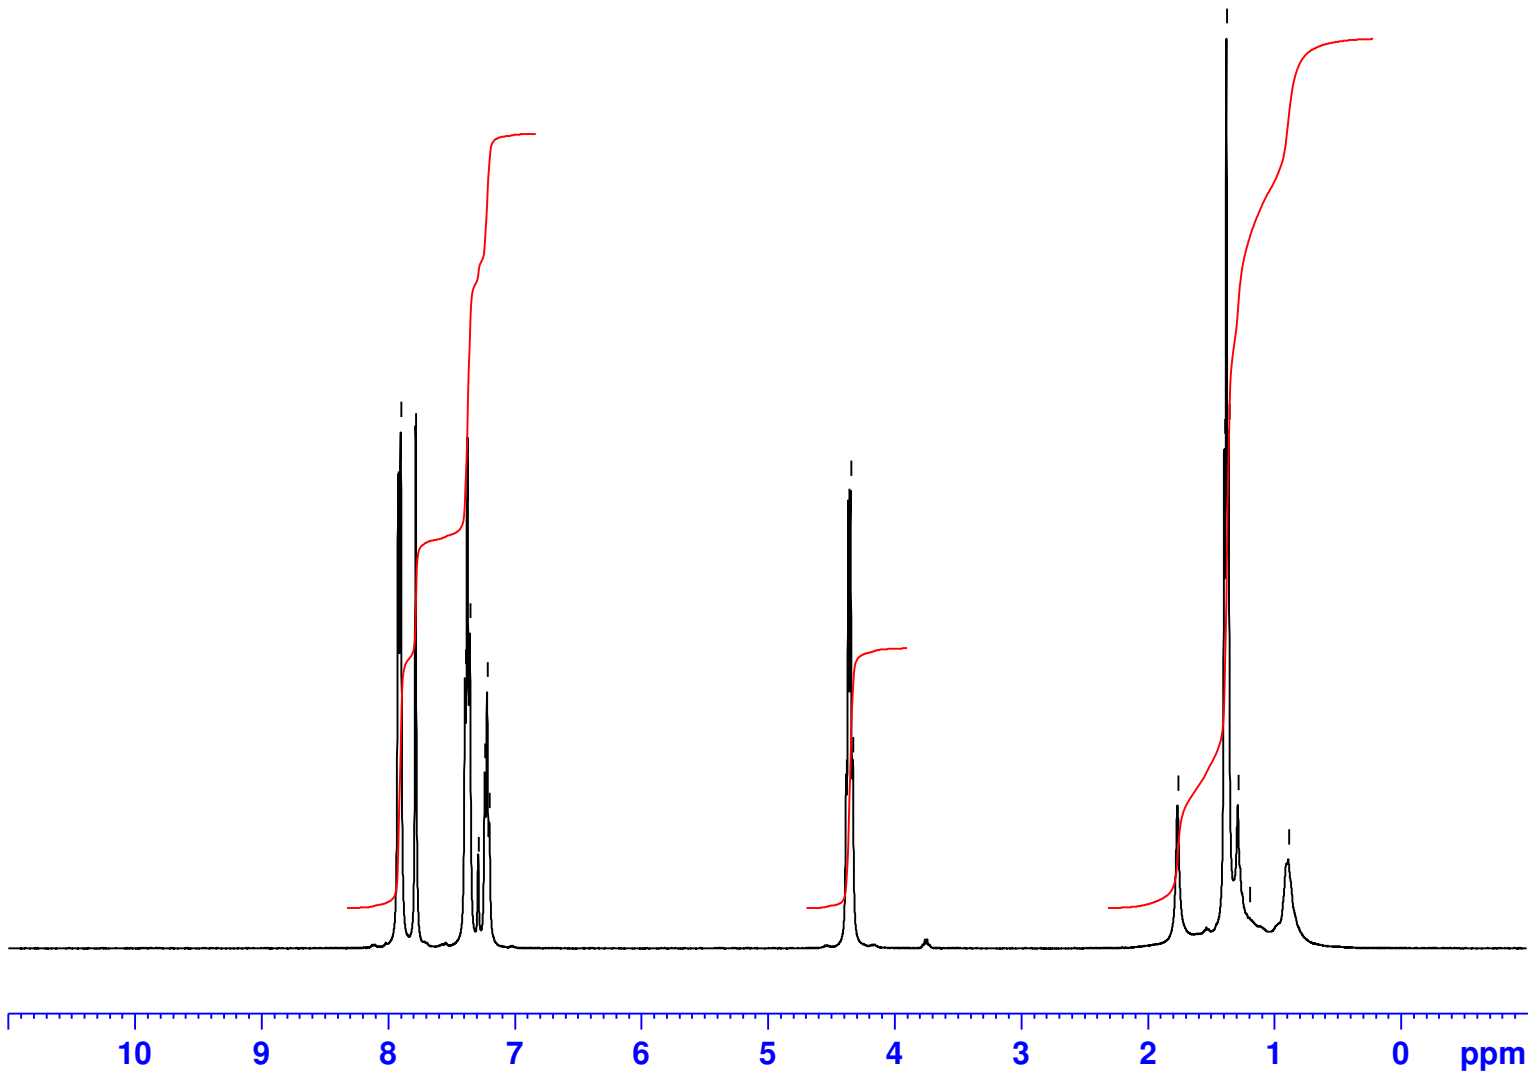

40.68
13.65
45.67