

TM-VI-171

7.998  
7.779  
7.730  
7.584  
7.567  
7.548  
7.517  
7.454  
7.435  
7.285  
7.205  
7.184  
6.627  
6.607

5.000

3.751  
3.734  
3.672

1.309  
1.276  
1.259  
1.242  
1.095


**Av-400C**

Current Data Parameters  
 NAME Nov18-2021  
 EXPNO 70  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20211118  
 Time 13.27  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB-  
 PULPROG zg30  
 TD 32768  
 SOLVENT CDCl3  
 NS 16  
 DS 2  
 SWH 8012.820 Hz  
 FIDRES 0.244532 Hz  
 AQ 2.0447233 sec  
 RG 199.33  
 DW 62.400 usec  
 DE 6.50 usec  
 TE 294.6 K  
 D1 1.00000000 sec  
 TD0 1

===== CHANNEL f1 =====  
 SFO1 400.2024012 MHz  
 NUC1 1H  
 P1 10.00 usec  
 PLW1 19.95299911 W

F2 - Processing parameters  
 SI 32768  
 SF 400.2000000 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00

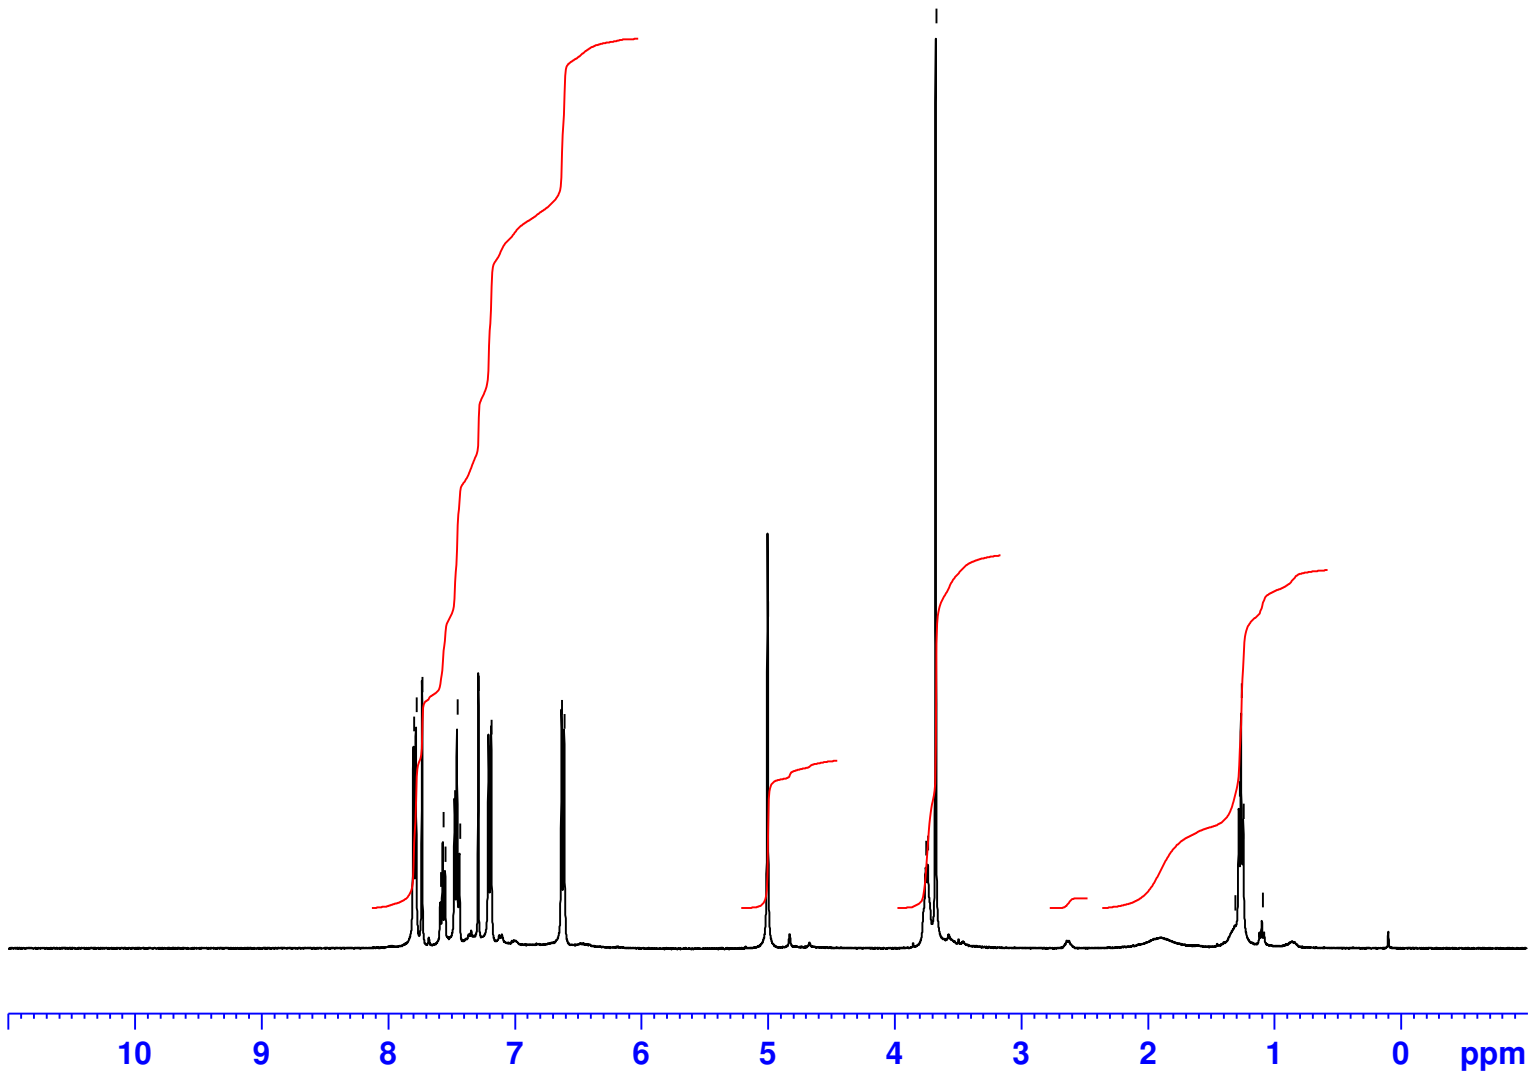

50.61  
8.58  
20.54  
0.58  
19.69