


**Av400B**

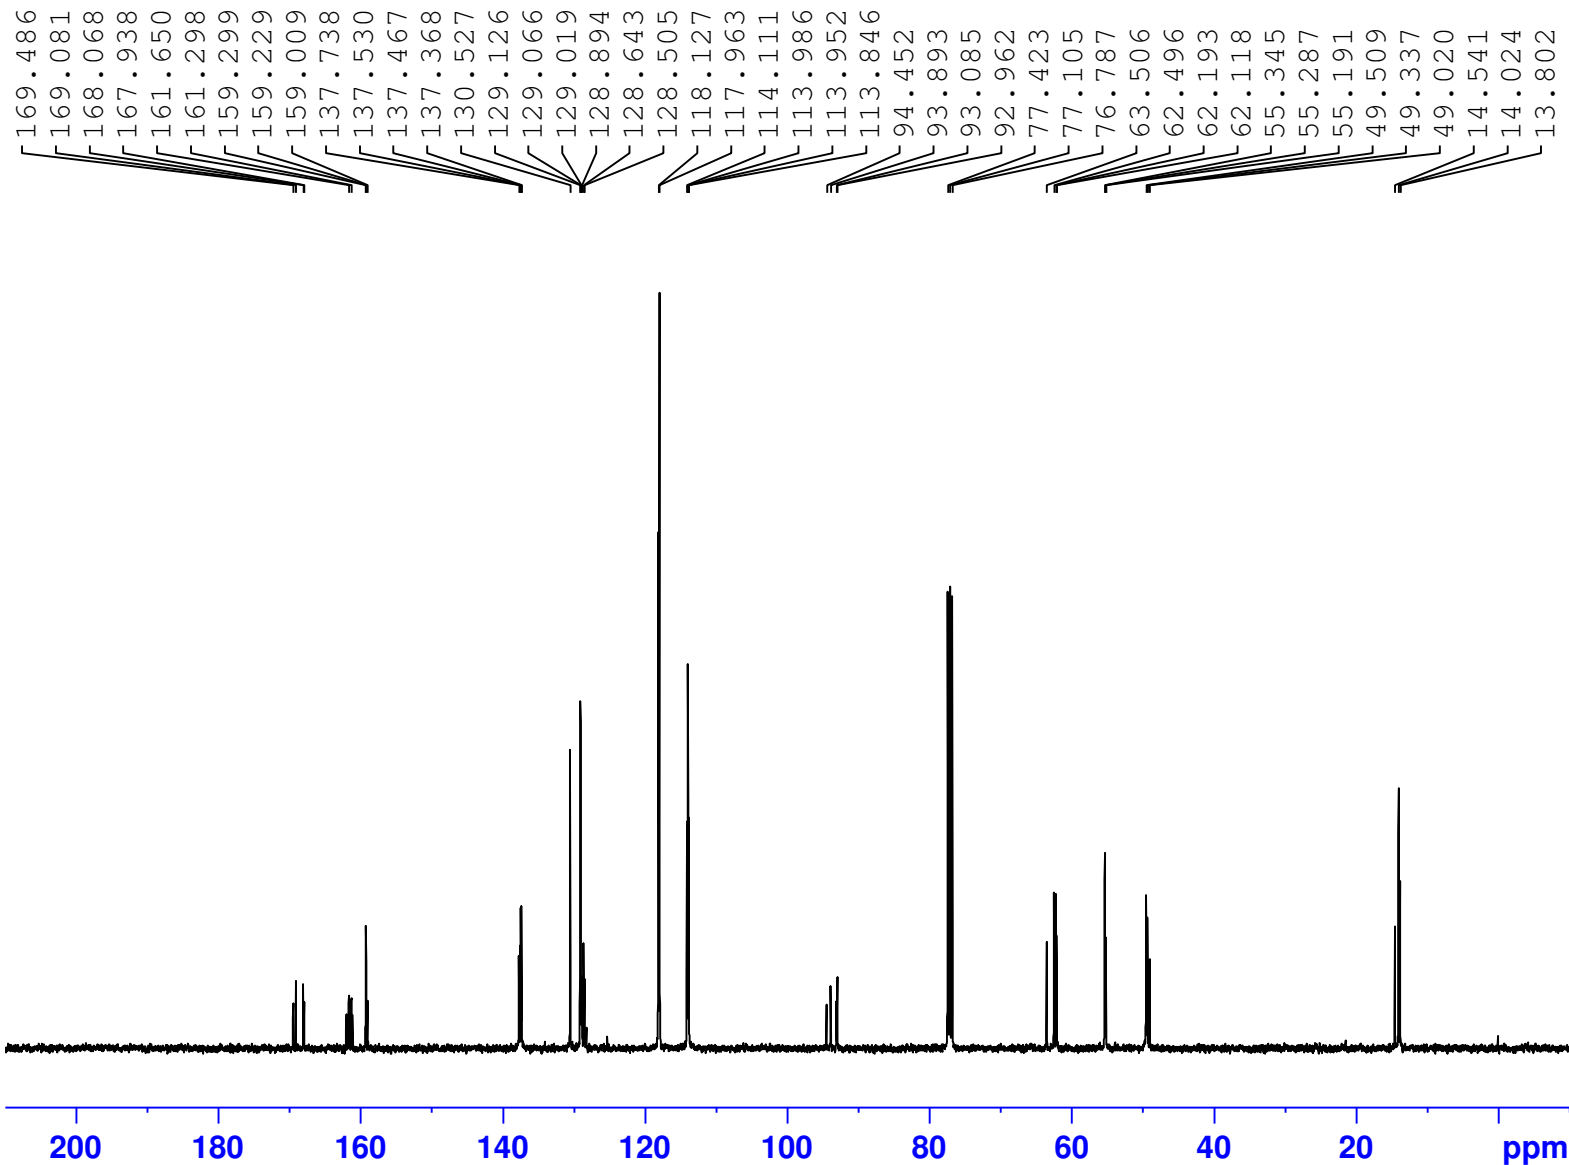

Current Data Parameters  
NAME Jun21-2022  
EXPNO 23  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220621  
Time 20.35  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zgpg30  
TD 32768  
SOLVENT CDC13  
NS 1200  
DS 4  
SWH 28409.092 Hz  
FIDRES 0.866977 Hz  
AQ 0.5767168 sec  
RG 199.76  
DW 17.600 usec  
DE 6.50 usec  
TE 296.0 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
TD0 1

=====  
CHANNEL f1  
SFO1 100.6716168 MHz  
NUC1 13C  
P1 9.25 usec  
PLW1 50.11899948 W

=====  
CHANNEL f2  
SFO2 400.3220016 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 19.95299911 W  
PLW12 0.22232001 W  
PLW13 0.18008000 W

F2 - Processing parameters  
SI 32768  
SF 100.6605440 MHz  
WDW EM  
SSB 0  
LB 2.00 Hz  
GB 0  
PC 1.20