


TM-VI-212, CDCl3, Cp2ZrCl + Ph-pyr.

**Av-400A**

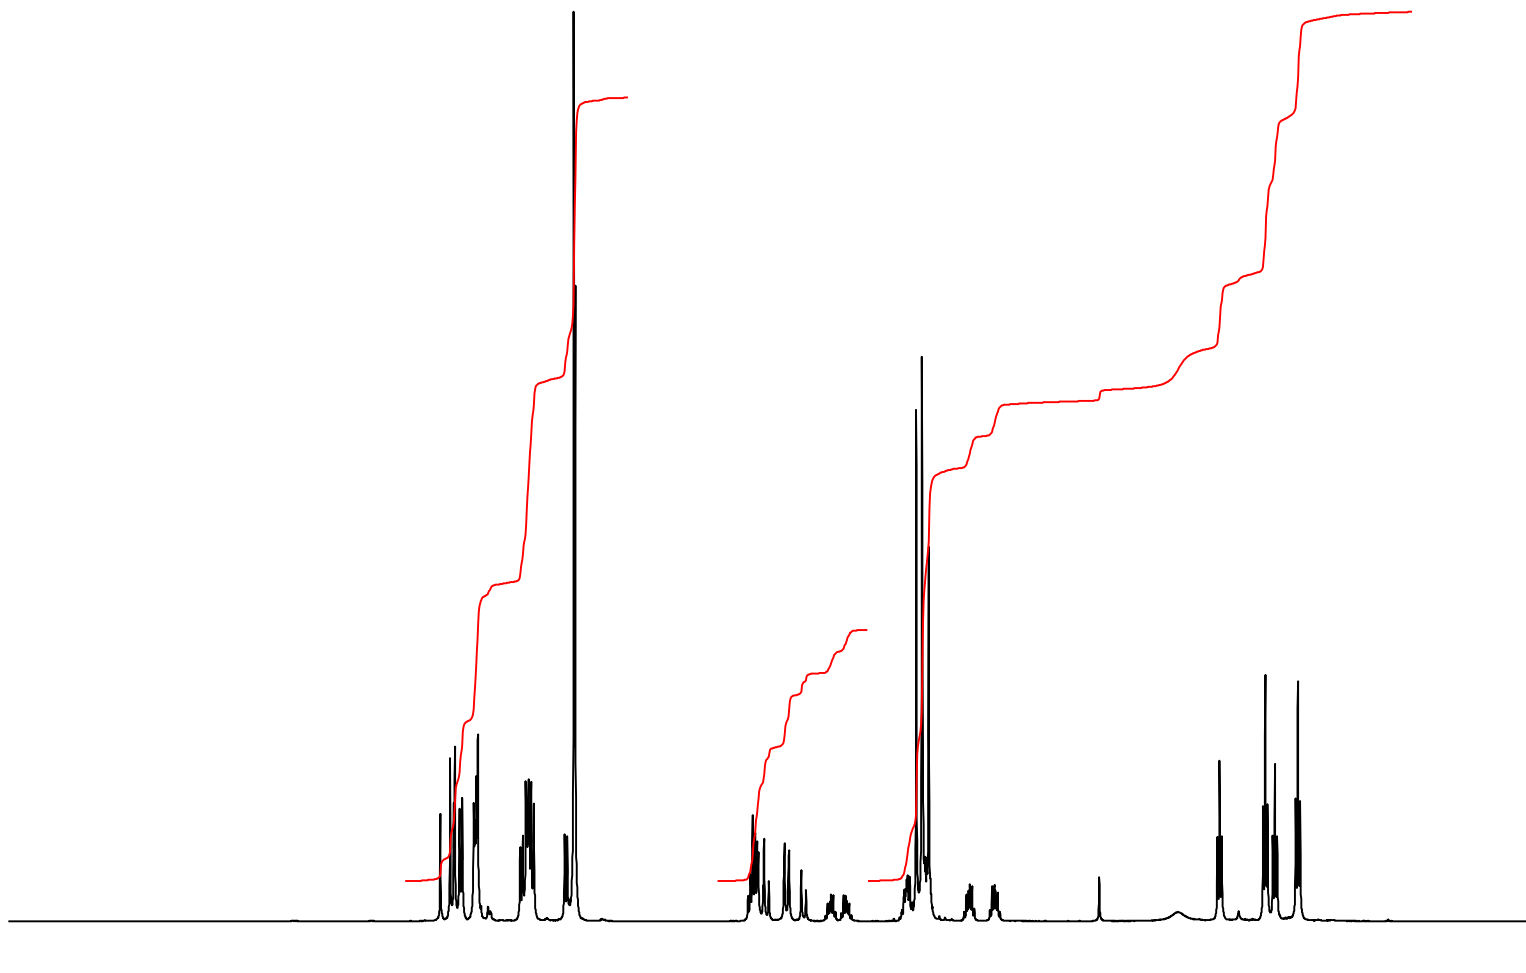

Current Data Parameters  
NAME Dec16-2021  
EXPNO 50  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20211216  
Time 12.01  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 2.0447233 sec  
RG 111.61  
DW 62.400 usec  
DE 6.50 usec  
TE 294.0 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 400.4124025 MHz  
NUC1 1H  
P1 11.25 usec  
PLW1 19.95299911 W

F2 - Processing parameters  
SI 16384  
SF 400.4100000 MHz  
WDW EM  
SSB 0  
LB 0.55 Hz  
GB 0  
PC 1.00

