


Av-400A

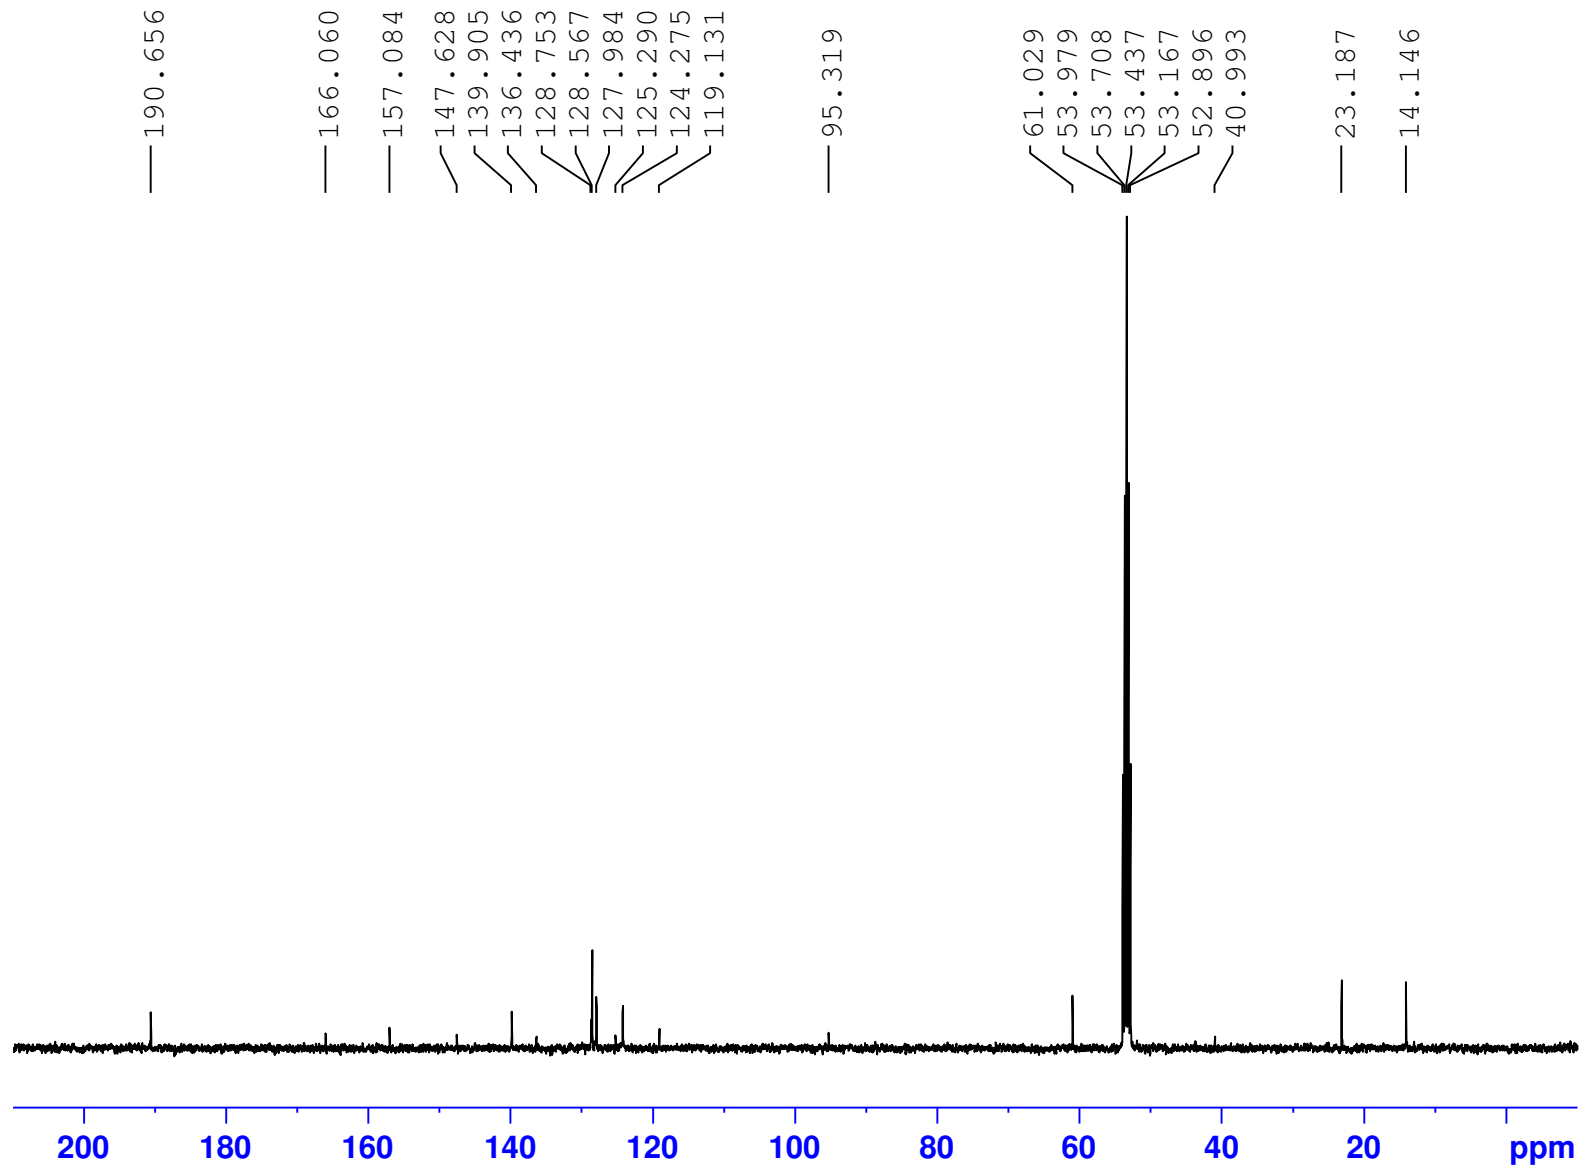

Current Data Parameters
 NAME Nov11-2021
 EXPNO 23
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20211111
 Time 21.26
 INSTRUM spect
 PROBHD 5 mm PABBO BB/
 PULPROG zgpg30
 TD 32768
 SOLVENT CD2Cl2
 NS 1200
 DS 4
 SWH 26315.789 Hz
 FIDRES 0.803094 Hz
 AQ 0.6225920 sec
 RG 207.33
 DW 19.000 usec
 DE 6.50 usec
 TE 295.1 K
 D1 1.00000000 sec
 D11 0.03000000 sec
 TD0 1

==== CHANNEL f1 =====
 SFO1 100.6942485 MHz
 NUC1 13C
 P1 9.60 usec
 PLW1 59.97900009 W

==== CHANNEL f2 =====
 SFO2 400.4119220 MHz
 NUC2 1H
 CPDPRG[2] waltz16
 PCPD2 90.00 usec
 PLW2 19.95299911 W
 PLW12 0.31176999 W
 PLW13 0.25253001 W

F2 - Processing parameters
 SI 16384
 SF 100.6831750 MHz
 WDW EM
 SSB 0
 LB 2.50 Hz
 GB 0
 PC 1.40