


TM-VI-158

Av-400A

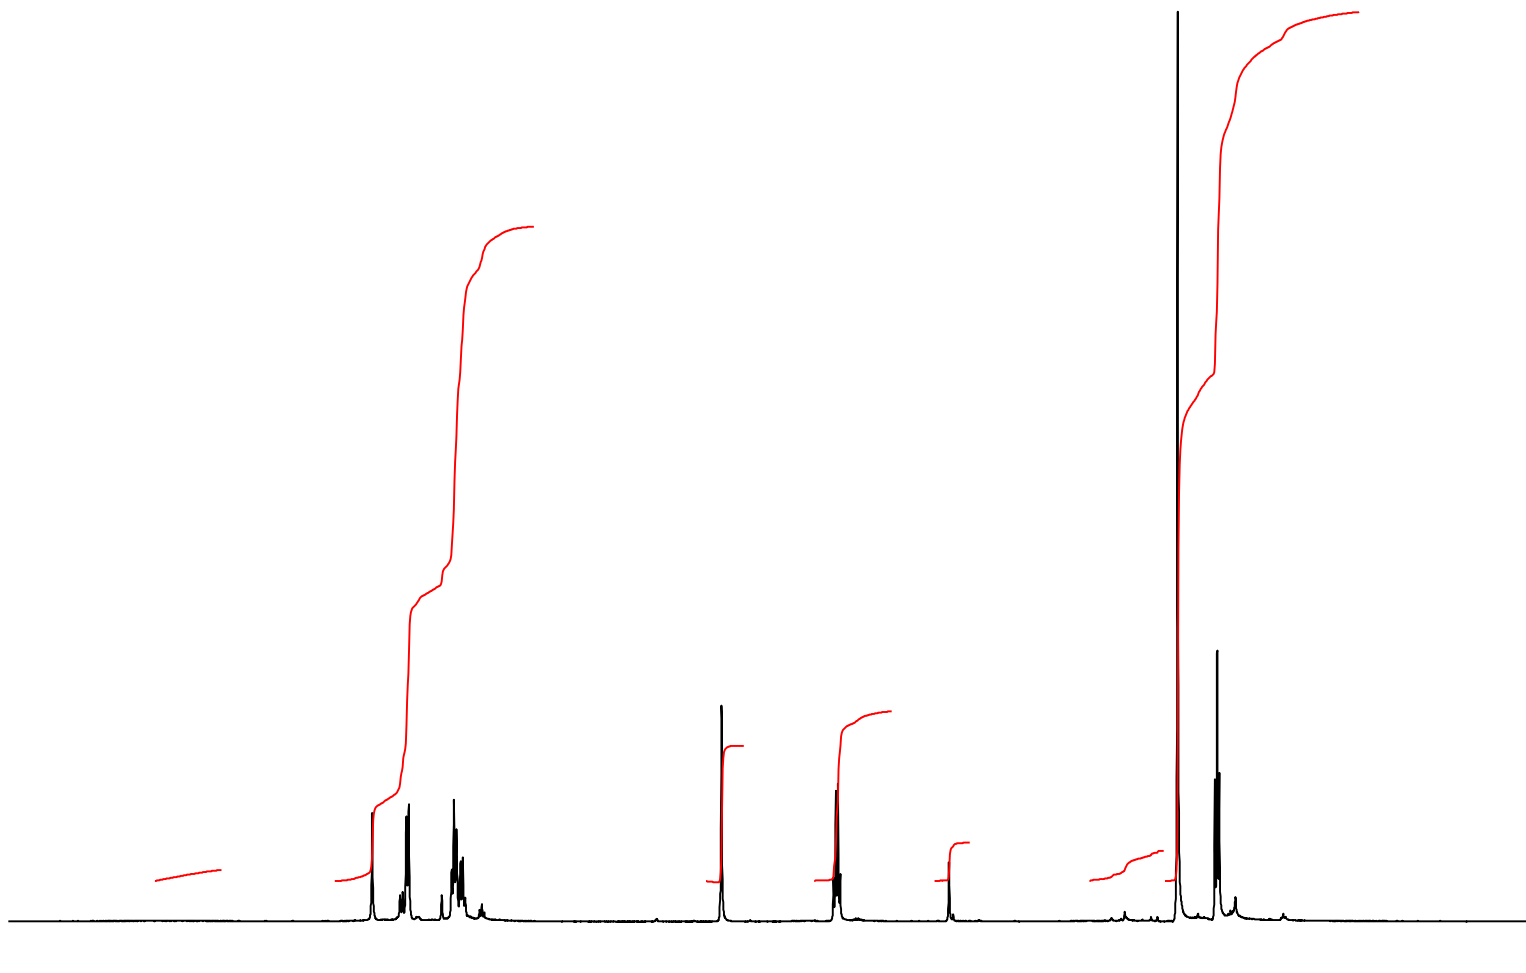

```
Current Data Parameters
NAME          Nov11-2021
EXPNO         20
PROCNO        1

F2 - Acquisition Parameters
Date_         20211111
Time          10.30
INSTRUM       spect
PROBHD        5 mm PABBO BB/
PULPROG       zg30
TD            32768
SOLVENT       CD2Cl2
NS            16
DS            2
SWH           8012.820 Hz
FIDRES        0.244532 Hz
AQ            2.0447233 sec
RG            207.33
DW            62.400 usec
DE            6.50 usec
TE            294.2 K
D1            1.00000000 sec
TD0           1

===== CHANNEL f1 =====
SFO1          400.4124025 MHz
NUC1           1H
P1             11.25 usec
PLW1          19.95299911 W

F2 - Processing parameters
SI            16384
SF            400.4100000 MHz
WDW           EM
SSB           0
LB            0.55 Hz
GB            0
PC            1.00
```

10 9 8 7 6 5 4 3 2 1 0 ppm

0.59 34.31 7.07 8.89 2.02 1.57 45.56