


TM-VI-191, CD3OD

**Av400B**

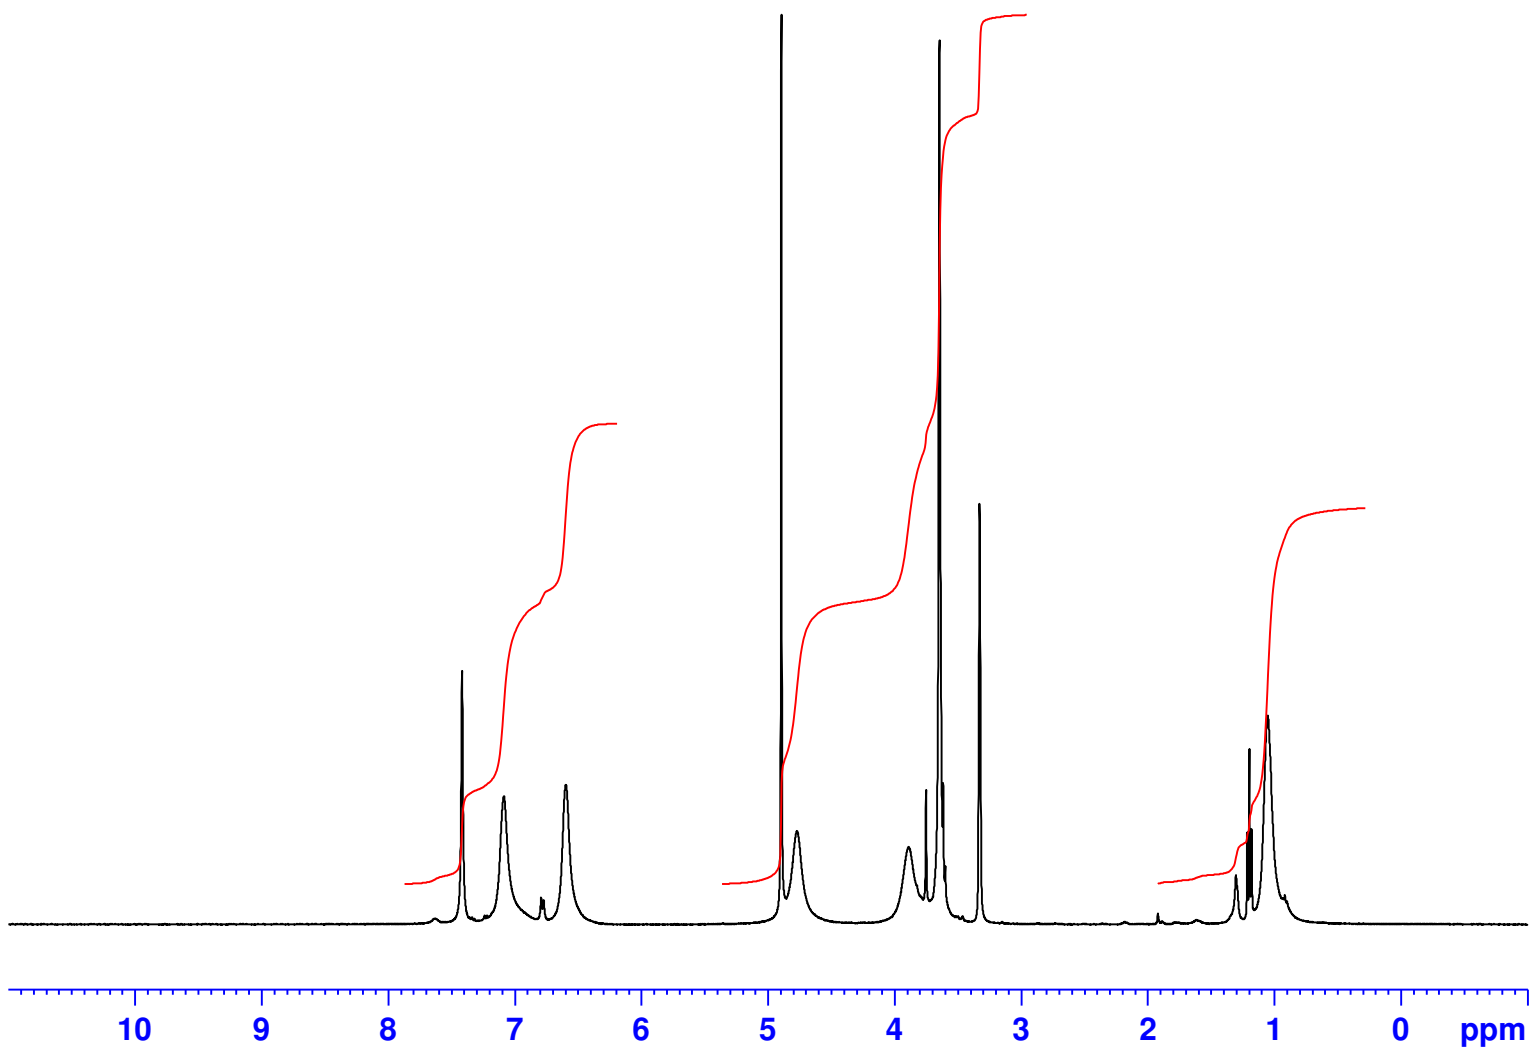

```
Current Data Parameters
NAME          Dec04-2021
EXPNO         20
PROCNO        1

F2 - Acquisition Parameters
Date_         20211204
Time          16.18
INSTRUM       spect
PROBHD        5 mm PABBO BB/
PULPROG       zg30
TD            32768
SOLVENT       MeOD
NS            16
DS            2
SWH           8012.820 Hz
FIDRES        0.244532 Hz
AQ            2.0447233 sec
RG            178.62
DW            62.400 usec
DE            6.50 usec
TE            294.7 K
D1            1.00000000 sec
TD0           1

===== CHANNEL f1 =====
SFO1          400.3224019 MHz
NUC1           1H
P1             11.00 usec
PLW1          20.00000000 W

F2 - Processing parameters
SI            32768
SF            400.3200000 MHz
WDW           EM
SSB           0
LB            0.30 Hz
GB            0
PC            1.00
```