



Auftraggeber Maulide  
hazh43 F2

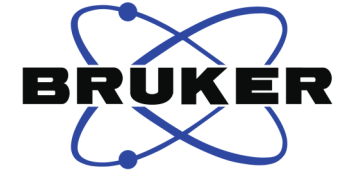

Current Data Parameters  
NAME 6Jul2419  
EXPNO 40  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190724  
Time 11.36 h  
INSTRUM spect  
PROBHD z126545\_0016 (  
PULPROG zg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 2  
SWH 12335.526 Hz  
FIDRES 0.376450 Hz  
AQ 2.6563926 sec  
RG 32  
DW 40.533 usec  
DE 12.00 usec  
TE 298.1 K  
D1 1.00000000 sec  
TD0 1  
SFO1 600.2537068 MHz  
NUC1 1H  
P1 12.25 usec  
PLW1 25.60000038 W

F2 - Processing parameters  
SI 65536  
SF 600.2500555 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

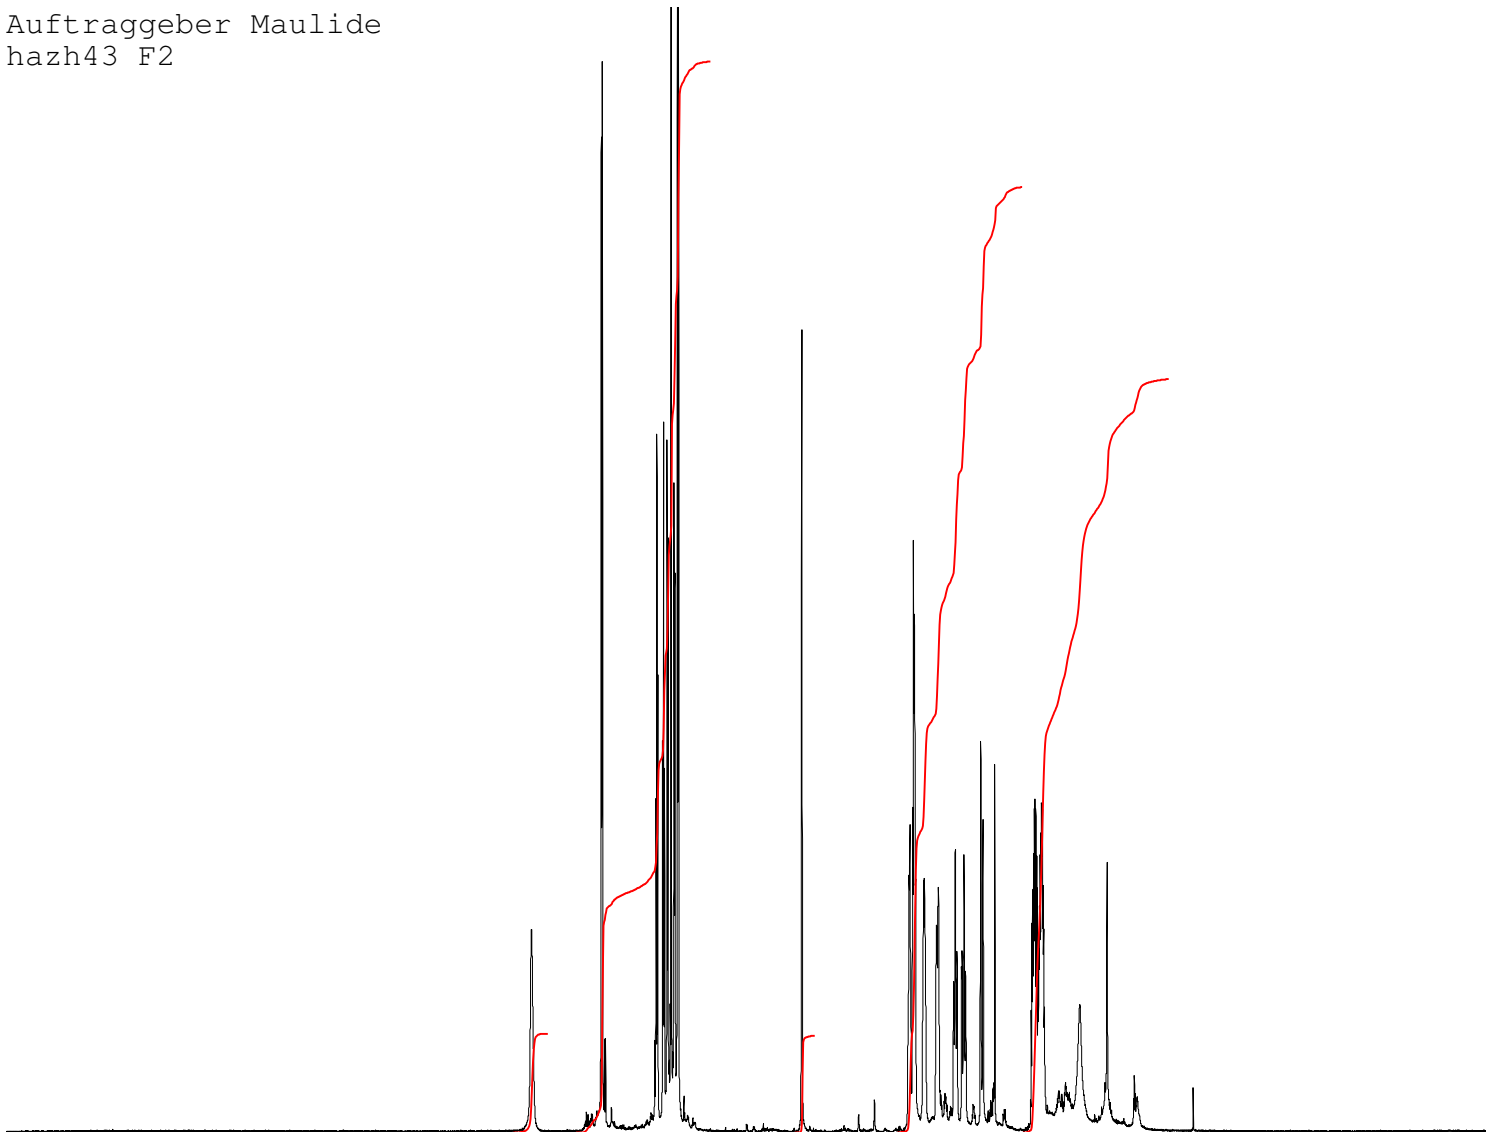

16 15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 ppm

3.3415  
36.1028  
3.2720  
31.8800  
25.4037