
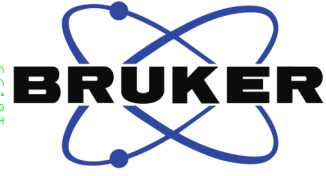


Auftraggeber Maulide

hazh_150

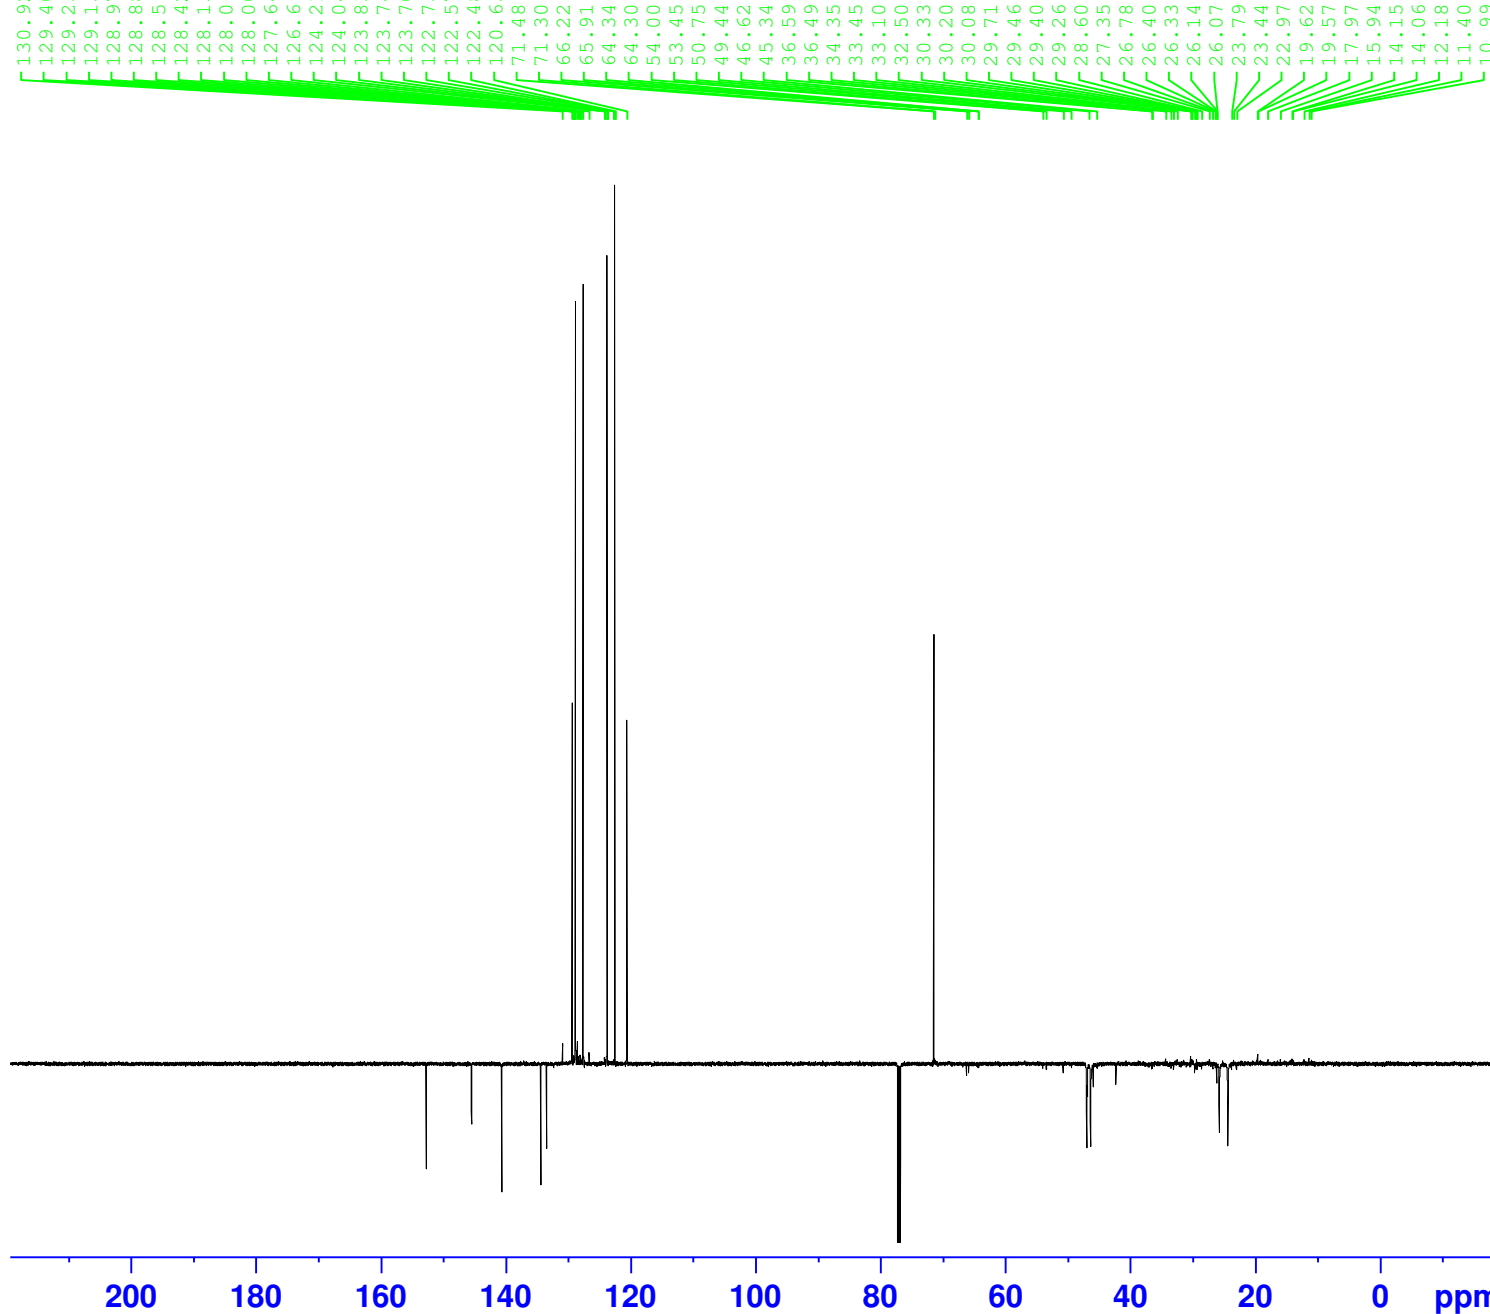

Current Data Parameters
NAME 6Sep3019
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190930
Time 8.17 h
INSTRUM spect
PROBHD Z126545_0016 (
PULPROG deptqgppp
TD 65536
SOLVENT CDC13
NS 300
DS 4
SWH 36057.691 Hz
FIDRES 1.100393 Hz
AQ 0.9087659 sec
RG 2050
DW 13.867 usec
DE 18.00 usec
TE 298.2 K
CNST2 145.0000000
D1 2.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
D16 0.00020000 sec
TD0 1
SFO1 150.9480754 MHz
NUC1 13C
P1 10.00 usec
P13 2000.00 usec
PLW0 0 W
PLW1 66.00000000 W
SPNAM[5] Crp60comp.4
SPOALS 0.500
SPOFFS5 0 Hz
SPW5 10.08399963 W
SFO2 600.2524010 MHz
NUC2 1H
CNST12 1.5000000
CPDPRG[2] waltz16
P0 18.38 usec
P3 12.25 usec
P4 24.50 usec
PCPD2 70.00 usec
PLW2 25.60000038 W
PLW12 0.78399998 W
GPNAM[1] SMSQ10.100
GPZ1 31.00 %
GPNAM[2] SMSQ10.100
GPZ2 31.00 %
GPNAM[3] SMSQ10.100
GPZ3 31.00 %
P16 1000.00 usec

F2 - Processing parameters
SI 131072
SF 150.9329825 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40