



Auftraggeber Maulide
hazh 104

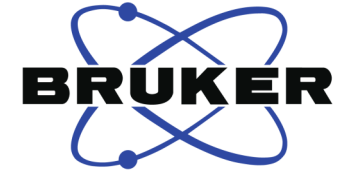

Current Data Parameters
NAME 6Aug2219
EXPNO 40
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190822
Time 13.52 h
INSTRUM spect
PROBHD z126545_0016 (
PULPROG zg30
TD 65536
SOLVENT CDC13
NS 16
DS 2
SWH 12335.526 Hz
FIDRES 0.376450 Hz
AQ 2.6563926 sec
RG 20.2
DW 40.533 usec
DE 12.00 usec
TE 298.1 K
D1 1.00000000 sec
TD0 1
SFO1 600.2537068 MHz
NUC1 1H
P1 12.25 usec
PLW1 25.60000038 W

F2 - Processing parameters
SI 65536
SF 600.2500488 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

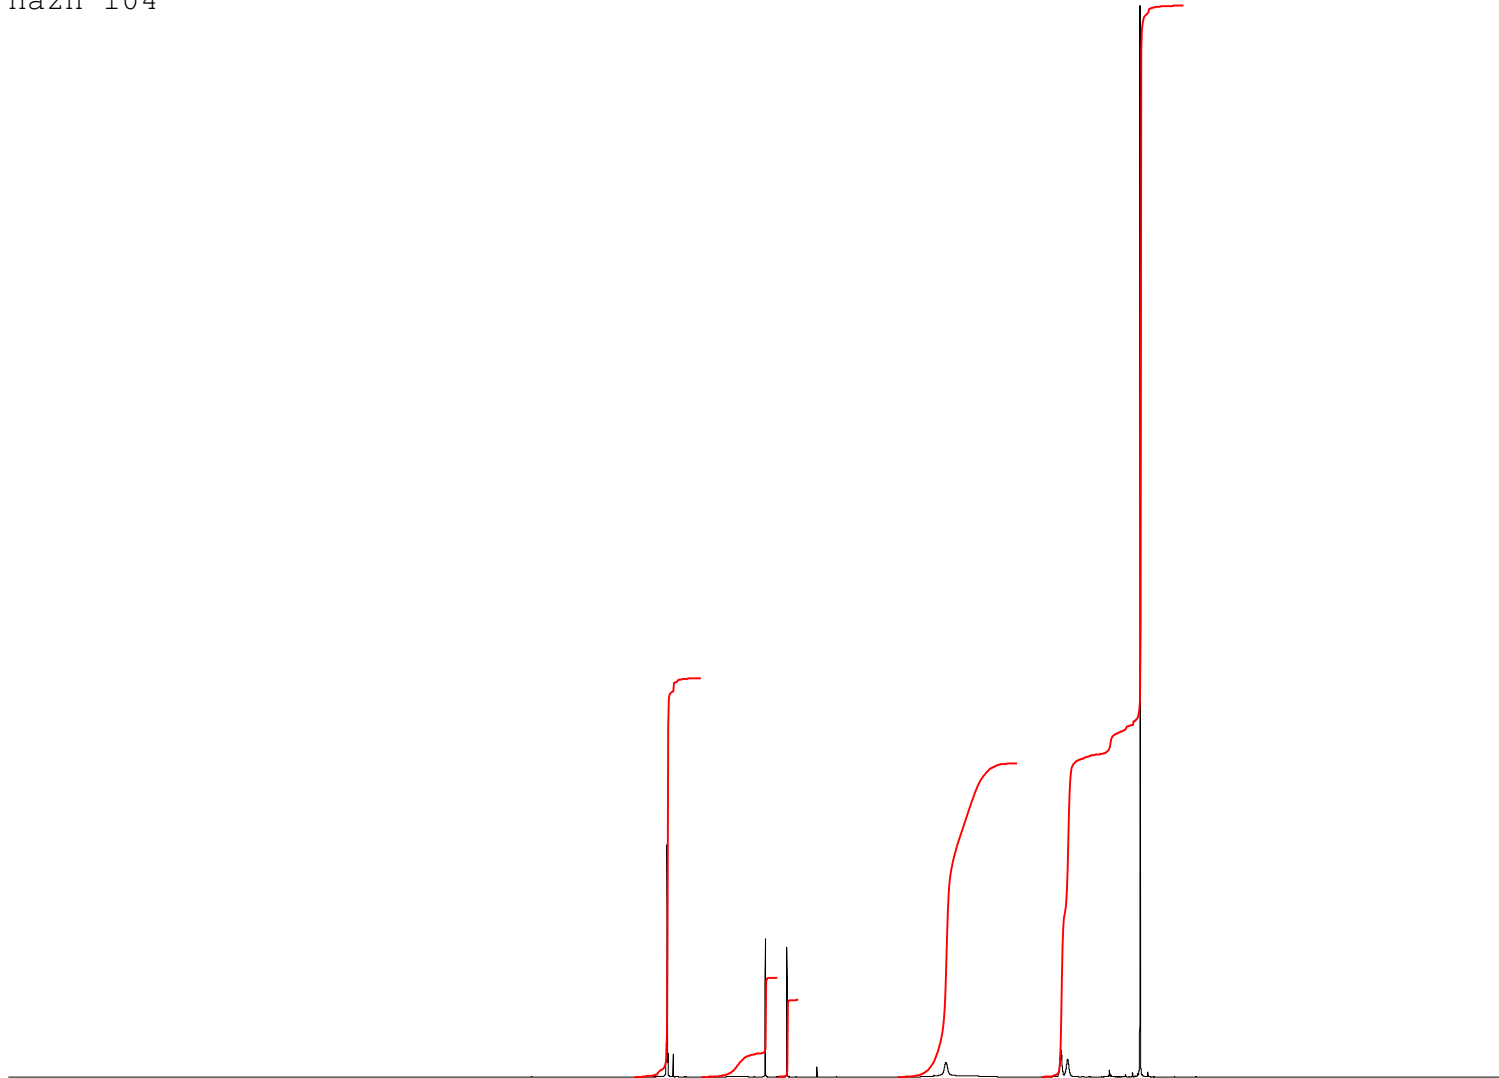

16 15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 ppm

20.3389
5.0814
3.9292
15.9844
54.6661